


Specifications NewTom 5G

Scan Unit

Acquisition Technique	Single Scan and Cone Beam Acquisition	
Scan parameters	Standard Modality:	18 s / 3,6 - 5,4 s
	Time / X-Ray Emission	360 degree rotation
Patient Positioning	Sitting / Supine	Motorized Patient Chair + laser
Weight and Dimension	Width	175 cm
	Depth (max)	230 cm (with patient's chair)
	Height	178 cm
	Gantry	58 cm
Total Weight	530 Kg (with patient's chair)	

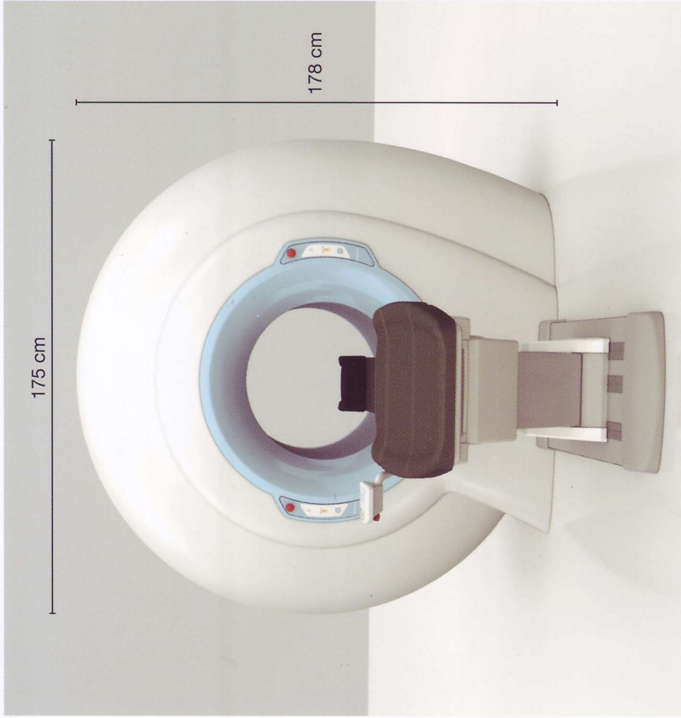


Multiples Scan Modes

Volume (d x h)	Standard Resolution (low dose)	Standard Resolution	Hi Resolution
18 x 16 cm	◆	◆	
15 x 12 cm	◆	◆	
12 x 8 cm	◆	◆	◆
8 x 8 cm	◆	◆	◆
6 x 6 cm			◆

Patient's Chair

Weight and Dimensioni	Width (max)	150 cm (footrest extended)
	Depth	70 cm
	Height	125 cm (backrest extended)
	Weight	120 Kg

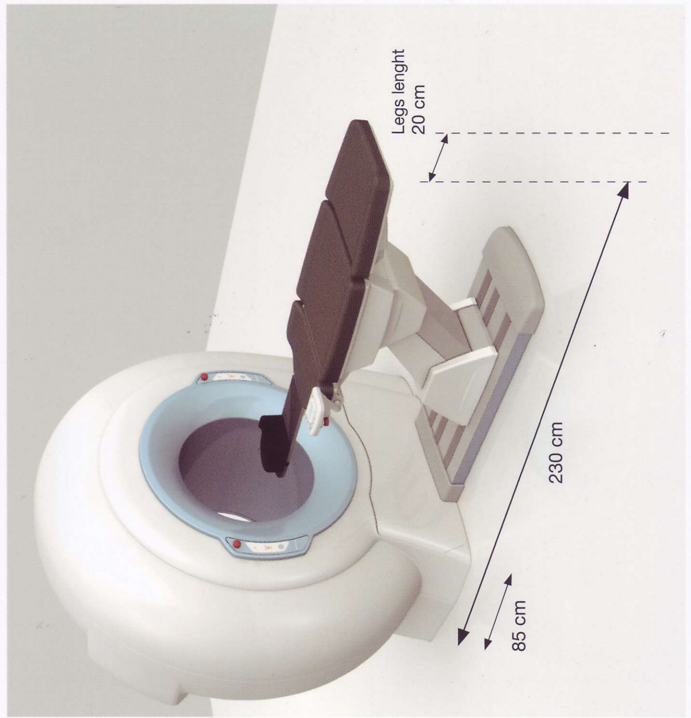

Specifications subject to change without prior notice.

QR srl

Via Silvestrini 20
37135 Verona

+39 045 8202727
+39 045 563500

info@qrverona.it
www.qrverona.it

CE
0051